



SHIELDskin XTREME™



A REVOLUTION IN GLOVE TECHNOLOGY

STERILE

BIO
CONTAMINATION
CONTROL

TECHNICAL
INFORMATION

SHIELDskin XTREME™
Sterile Latex 400 DI+

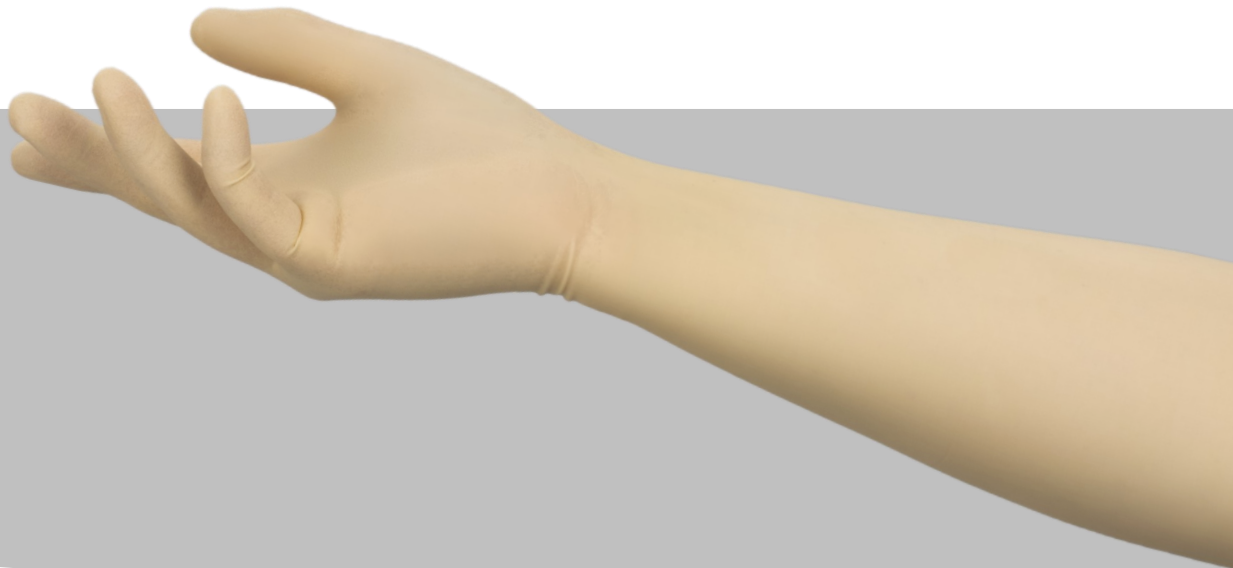

STERILE

BIO
CONTAMINATION
CONTROL

DI+

HIGH
CONTAMINATION
CONTROL

- ⇒ Powder-free triple DI washed hand-specific extra length (400 mm/ 15.7") sterile natural rubber latex cleanroom gloves.
- ⇒ Personal Protective Equipment Category III (PPE - Complex Design) according to Regulation (EU) 2016/425.
- ⇒ Fully compliant to the latest EU PPE norms relating to protective gloves against chemicals, micro-organisms and viruses.


DESCRIPTION	
FORMULATION	Natural rubber latex (<i>Hevea brasiliensis</i>).
DESIGN	Natural colour, hand-specific, beaded cuff, fully textured.
PACKAGING	1 pair per PE peel pouch - 20 pouches per sealed poly bag - 8 poly bags per PE bag per carton.

SIZES	5.5	6.0	6.5	7.0	7.5	8.0	8.5	9	10
CODES	69 5771	69 5772	69 5773	69 5774	69 5775	69 5776	69 5777	69 5778	69 5779

STANDARDS	
CE REGISTRATION	PPE Category III (Complex Design) - Regulation (EU) 2016/425. Notified Body No 0598: SGS Fimko Oy, Helsinki - FINLAND.
EU PPE NORMS	EN 420:2003+A1:2009, ISO 374-1:2016+A1:2018, EN 374-2:2014, ISO 374-4:2013, ISO 374-5:2016, EN 16523-1:2015+A1:2018 and ISO 16604:2004 Procedure B.
EU MDD NORMS ¹	EN 455-1:2000, EN 455-2:2015, EN 455-3:2015 and EN 455-4:2009.
USA STANDARDS	ASTM D3767-03 (2014), ASTM D573-04 (2015), ASTM D412-16, ASTM D5712-15 and IEST-RP-CC005.4 (2013).
OTHER STANDARDS	ISO 11137-2:2015, ISO10993-10:2010.

¹With reference to Council Directive 93/42/EEC for Medical Devices

QUALITY	
QUALITY ASSURANCE	Production management in accordance with ISO 9001:2015 and ISO 13485:2016.
TECHNOLOGY	uniSHIELD™ single-walled protection to offer an ideal compromise between comfort and protection. Compatible with sterile processing environments due to paperless packaging and multiple post leaching of gloves (triple washed in deionised water).

DOCUMENTATION			
DECLARATION OF CONFORMITY	These documents can be freely downloaded from the product page on our website: www.shieldscientific.com .		
EU TYPE EXAMINATION CERTIFICATE			For an easy access, scan the QR code.
PRODUCT INSERT			
CERTIFICATE OF CONFORMANCE	To access CoC and Col, you need to be registered. Please contact us at info@shieldscientific.com or call your SHIELD Scientific representative.		
CERTIFICATE OF IRRADIATION			

A REVOLUTION IN GLOVE TECHNOLOGY

PHYSICAL PROPERTIES



NOMINAL THICKNESS		mm ²	mil	Norm
⇒	Finger	0.20	7.9	ASTM D3767-03 (2014)
⇒	Palm	0.18	7.1	
⇒	Cuff	0.13	5.1	

² Thickness (+/- 0.03 mm)

LENGTH		Minimum	Typical	Norm
⇒	From middle finger tip to edge of cuff	400 mm / 15.7"	405 mm / 15.9"	EN 420:2003+A1:2009

STRENGTH PROPERTIES	Force at break (spec.)		Ultimate elongation (spec.)	Force at break (typical)	Norm
	⇒	Before aging	≥ 9.0N 18 Mpa	≥ 700%	
⇒	After aging	≥ 6.0N 14 Mpa	≥ 500%	12.0N	

FREEDOM FROM HOLES		Performance	Norm
⇒	Acceptable Quality Level (AQL)	< 0.65 ³ - Level 3	EN 374-2:2014

³ AQL as defined per ISO 2859-1:1999 for sampling by attributes.

RISKS	Description	Norm
MICRO-ORGANISMS	1000 ml water test. Performance level 3, AQL < 0.65 (inspection level G1).	EN 374-2:2014
VIRUSES ⁴	Viral penetration test using Phi-X174 bacteriophage according to ISO 16604:2004 Procedure B.	ISO 374-5:2016
CHEMICALS ⁴	<u>Performance</u> : Type B (KPT). <u>Permeation</u> : Extensively tested. Online chemical resistance guide on www.shieldscientific.com . <u>Degradation</u> : Tested for determination of resistance to degradation by chemicals.	ISO 374-1:2016+A1:2018 EN 16523-1:2015+A1:2018 EN 374-4:2013

⁴ For PPER compliance, ≥ 40 cm gloves are palm and cuff tested for permeation, degradation and viral penetration.

CLEANLINESS PROPERTIES

PARTICLES	Specification	Typical value	Test method
Particles/cm ² ≥ 0.5µm	<1 200 particles	1 100 particles	IEST-RP-CC005.4

EXTRACTABLES (ION)	Specification (µg/cm ²)	Typical value (µg/cm ²)	Test method
Ammonium (NH ₄)	0.100	0.050	IEST-RP-CC005.4
Bromide (Br)	0.050	<0.008	
Calcium (Ca)	0.500	0.390	
Chloride (Cl)	0.200	0.100	
Fluoride (F)	0.010	<0.008	
Magnesium (Mg)	0.010	<0.008	
Nitrate (NO ₃)	0.400	0.210	
Nitrite (NO ₂)	0.050	<0.008	
Phosphate (PO ₄)	0.050	<0.008	
Potassium (K)	0.050	0.020	
Sodium (Na)	0.050	0.020	
Sulphate (SO ₄)	0.050	0.015	

EXTRA TESTS	Description	Test method
STERILITY	Terminally sterilized by gamma irradiation to Sterility Assurance Level (SAL) of 10 ⁻⁶ (ISO 11137-2:2015).	
ENDOTOXINS	Low Endotoxin content at < 20 EU/pair demonstrated by Limulus Amoebocyte Lysate (LAL) kinetic turbidimetric test.	EN 455-3:2015
NVR	Maximum 30 mg/g.	IEST-RP-CC005.4
FTIR	Non-detectable levels of silicone, amide and DOP.	IEST-RP-CC005.4

ALLERGIES	
BIO-COMPATIBILITY	Demonstrated by skin irritation and sensitization tests in accordance with ISO 10993-10:2010.
ACCELERATORS	Free of Thiazoles and Thiurams. These chemical accelerators are excluded from the manufacturing process.
CHEMICAL ALLERGENS	Non-detectable levels using aqueous solution extraction (Phosphate buffered solution) and High Performance Liquid Chromatography (HPLC) assay method for quantitative analysis.
LATEX PROTEIN	≤ 50 µg/g as per Modified Lowry Method (EN 455-3:2015/ASTM D5712-15). Typical: ≤ 30 µg/g as per Modified Lowry Method.



Dr. Willem Dreeslaan 1 • 6721 ND Bennekom • The Netherlands
Phone +31 (0)317 700 202 • Fax +31 (0)318 503 742
E-mail: Info@shieldscientific.com

WWW.SHIELDSCIENTIFIC.COM